










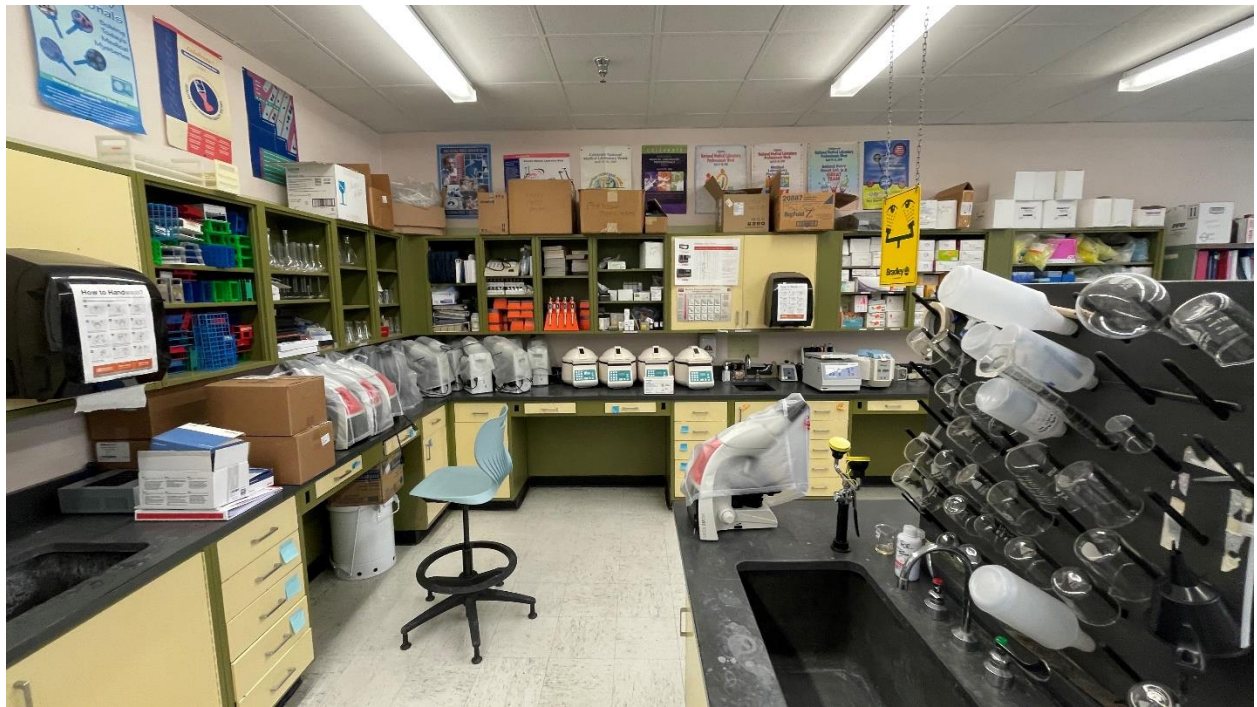


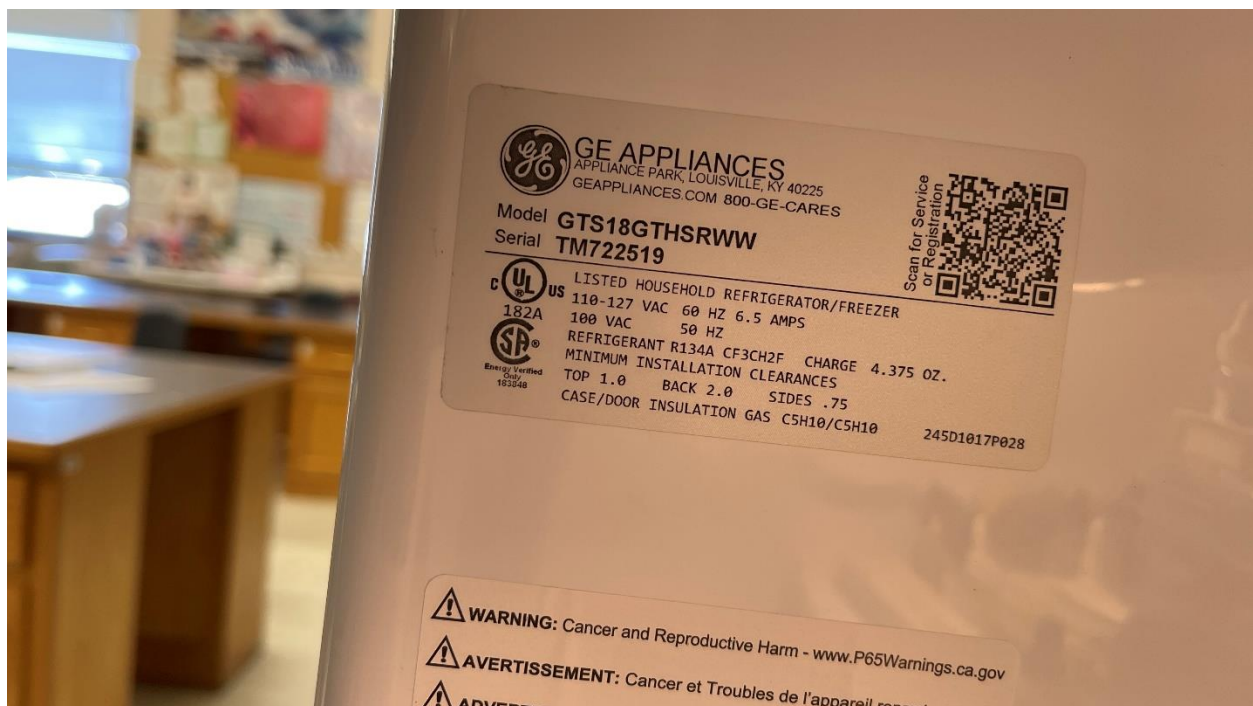

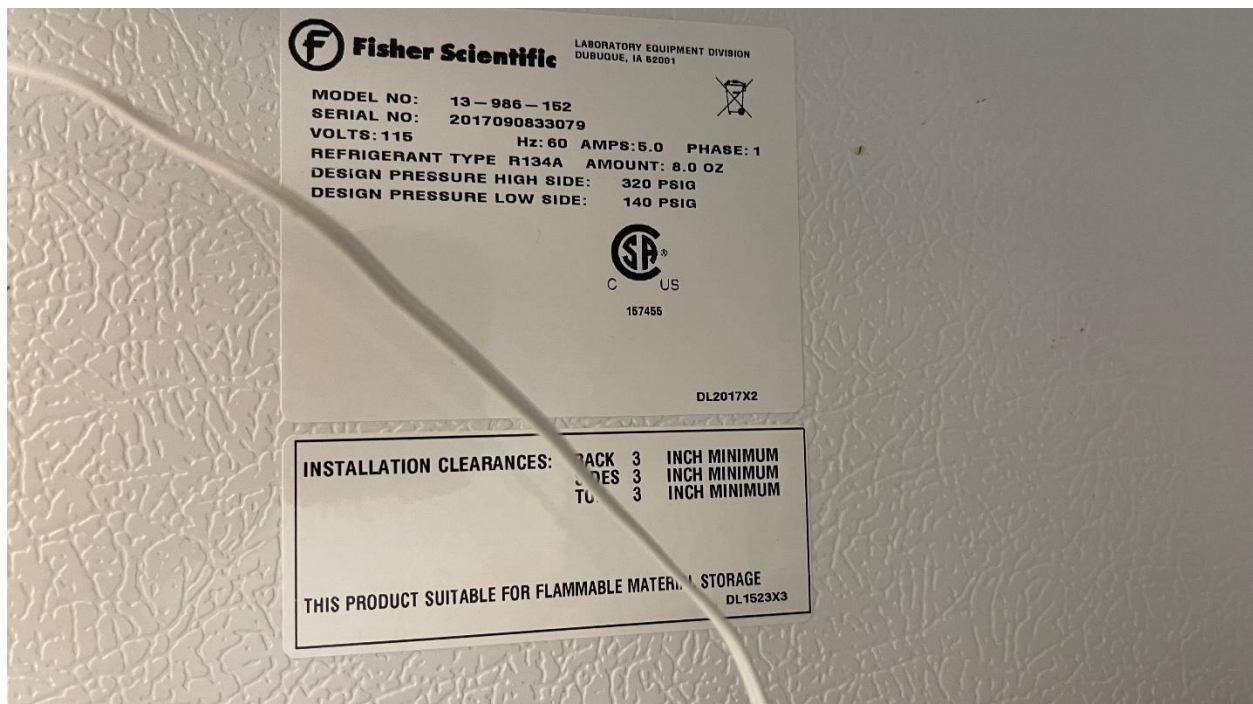

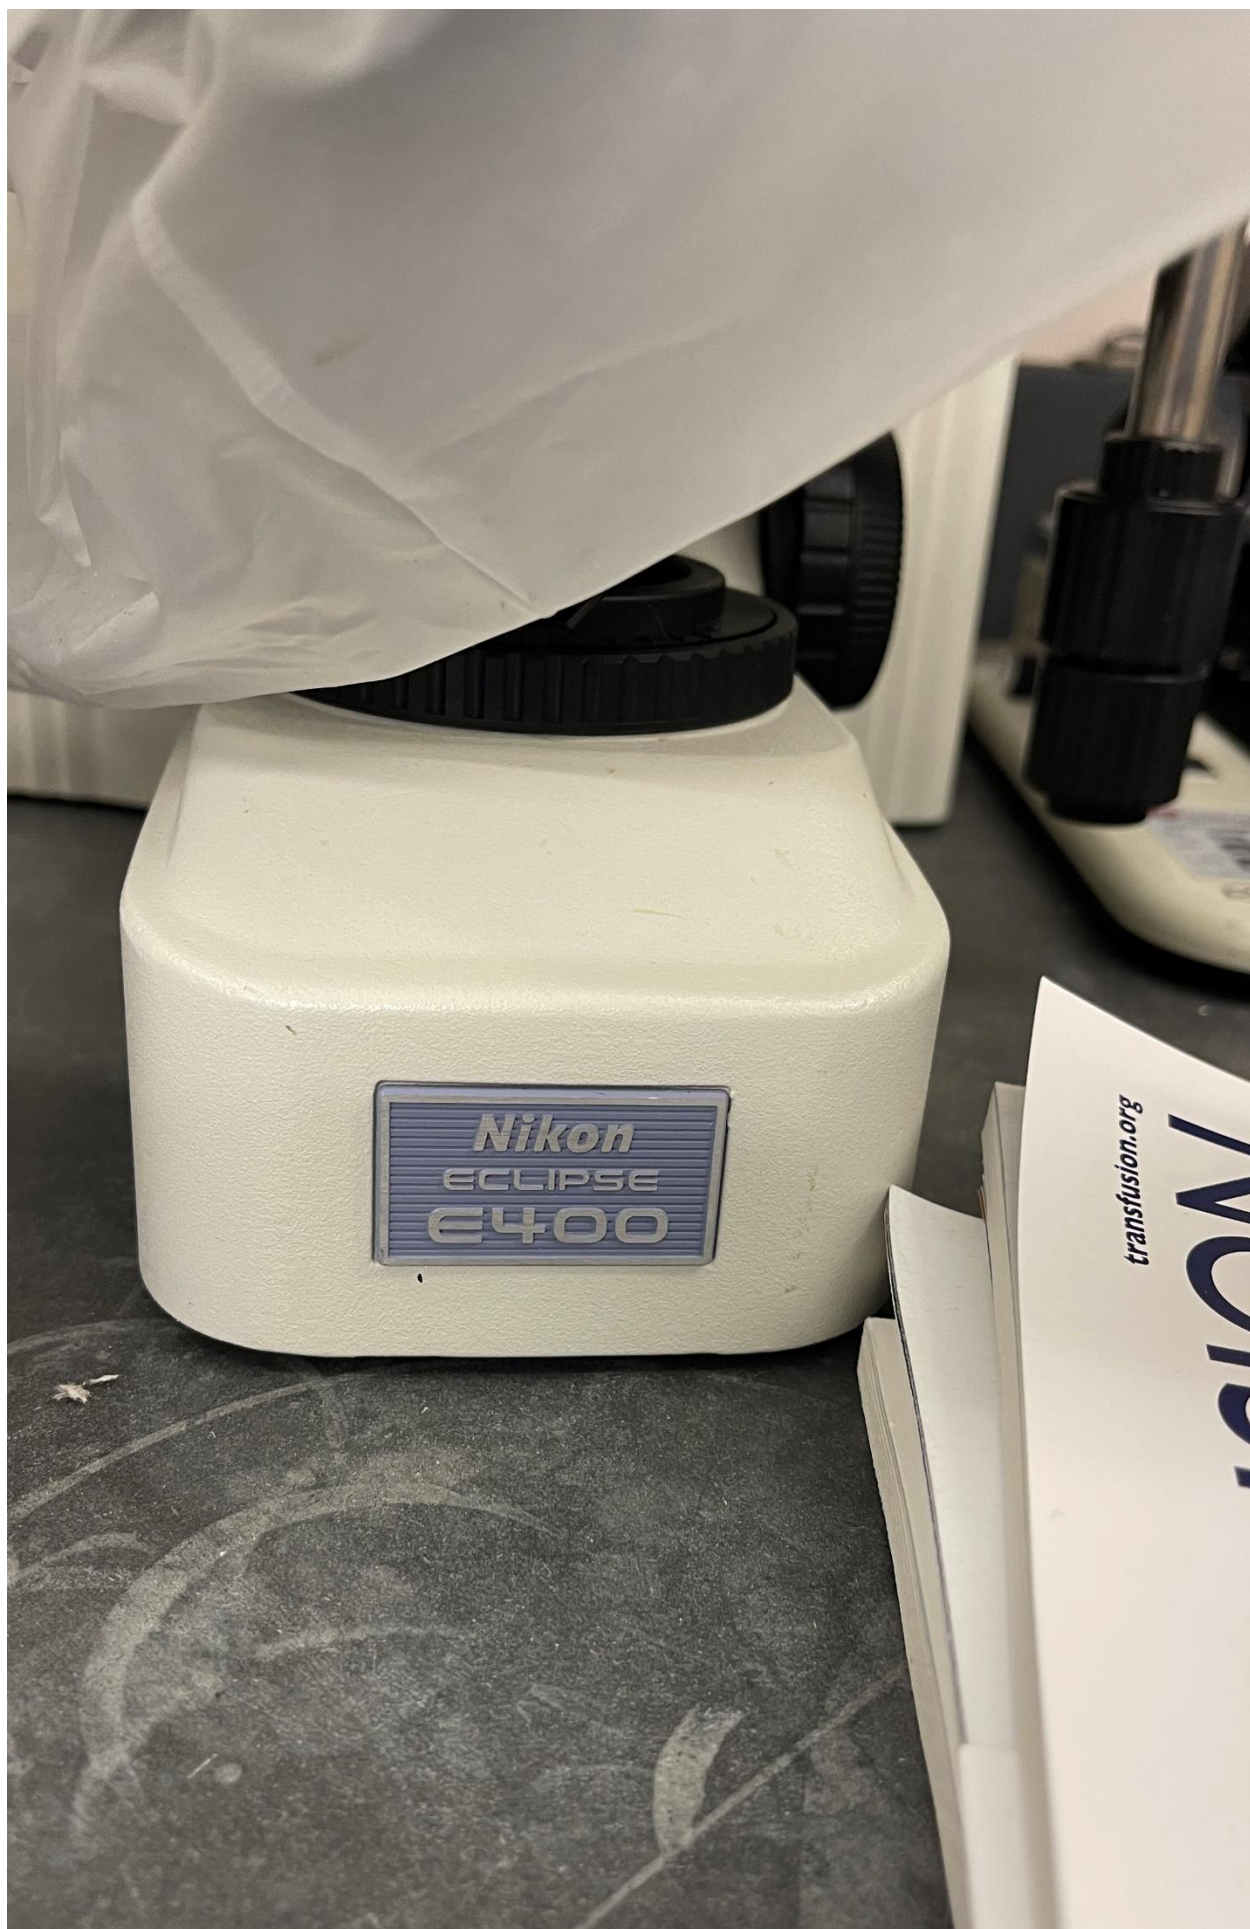

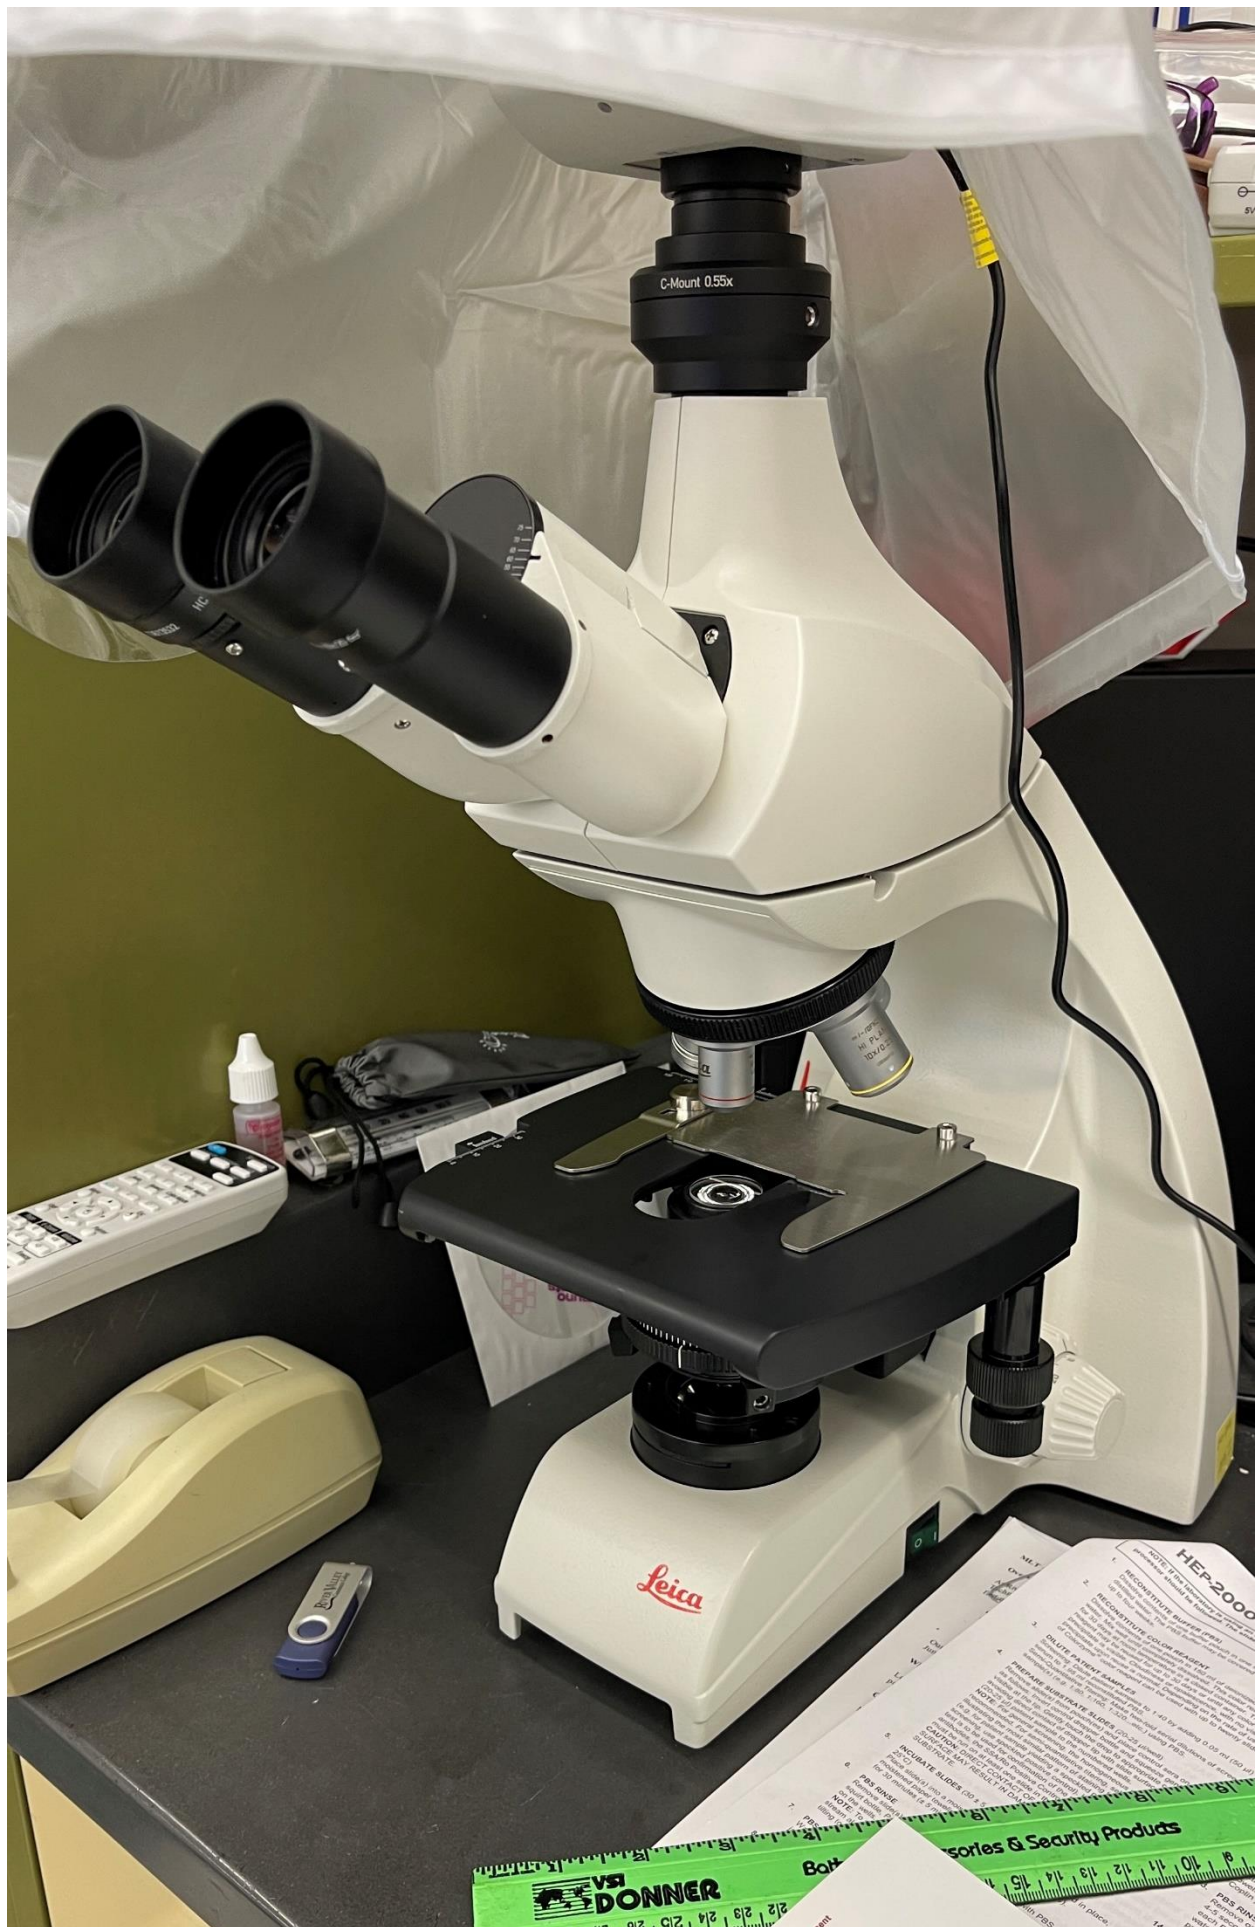

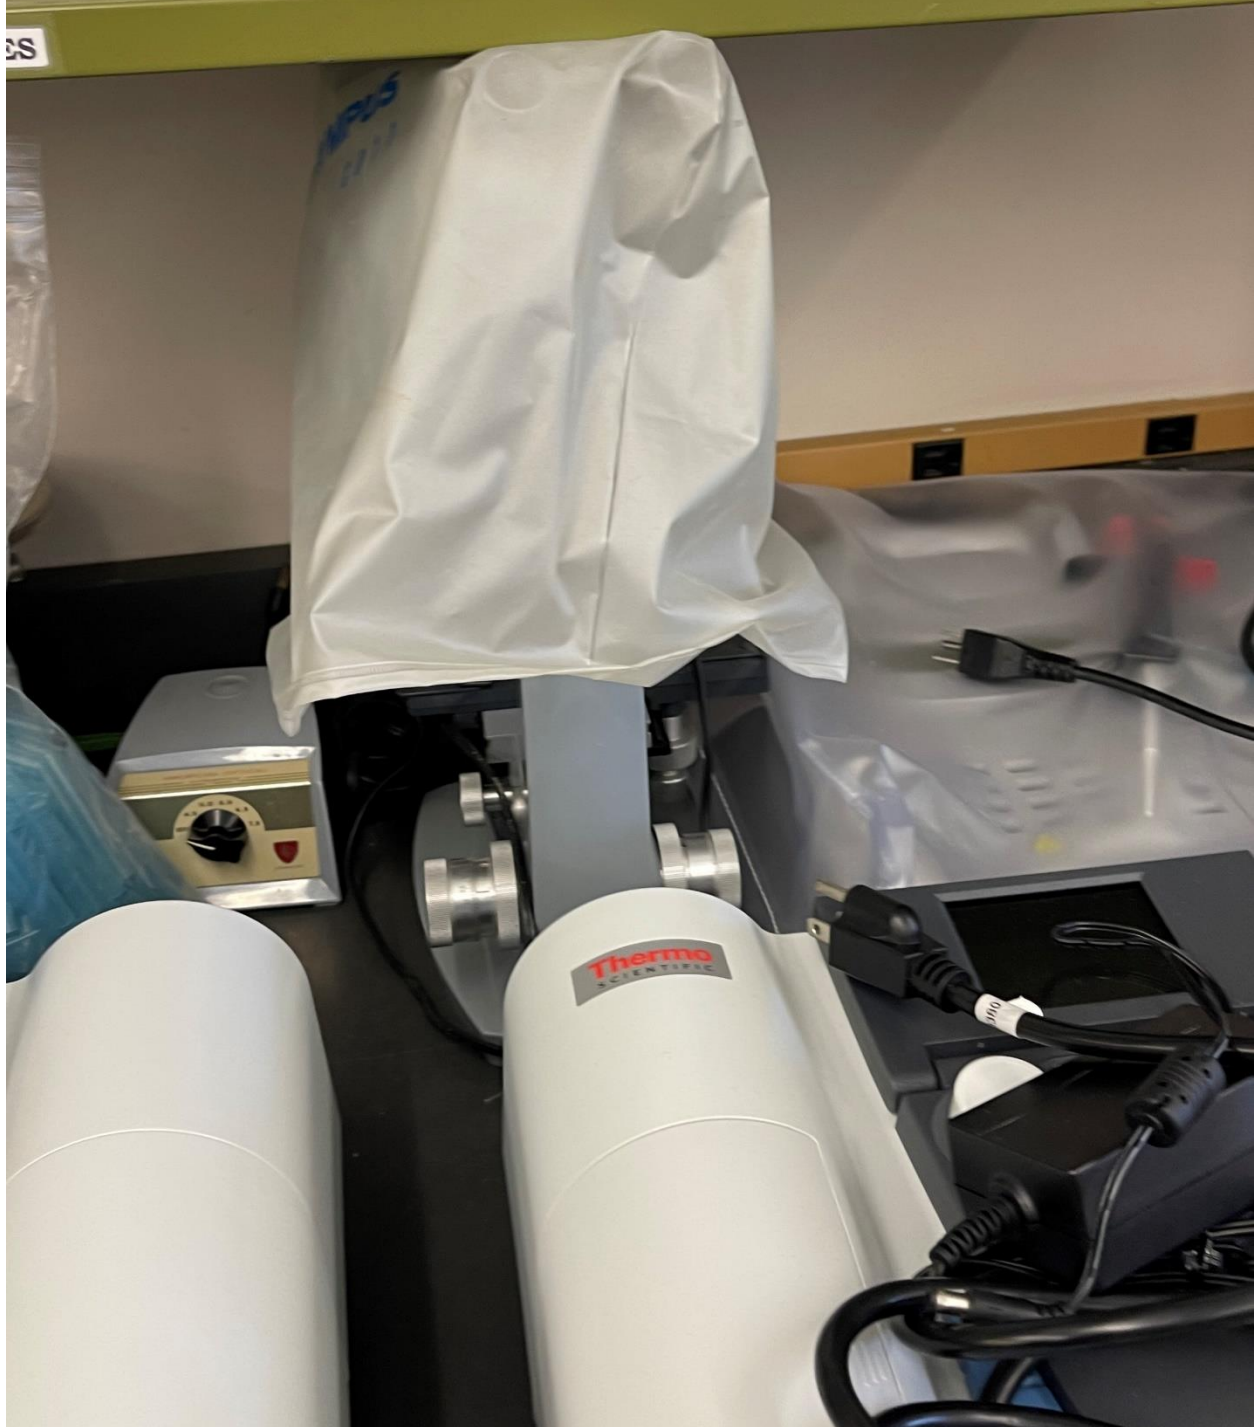















 **POINTE 180**  **CHEMISTRY ANALYZER**

Digital display area



YES

ABS 1	STND 2	FAC 3	AUX —
----------	-----------	----------	----------

PGM 4	%ABS 5	DUP 6	Paper
----------	-----------	----------	-------

RATE 7	FILT 8	TEMP 9	Clear
-----------	-----------	-----------	-------

NO

BLANK 0	TEST •	Lamp	Enter
------------	-----------	------	-------

Thermo

ELECTRON CORPORATION
MILFORD, MA 01757



CENTRA-CL2
MODEL

42618076

SERIAL NUMBER

120

VOLTS AC

4.0

AMPERES

60

HERTZ

MADE IN CHINA

YR 2005

HYP
EMP#



OUT
OF
SERVICE

Thermo
ELECTRON CORPORATION

IEC
CENTRA CL2
Centrifuge

RPM X 1000




 **VWR INTERNATIONAL**

TYPE: **Clinical 200** REF 306.00 V40
SN 68165069 2016

MAX. DREHZAHL: 6000 1/min. KIN. EN.: 2427 Nm
U/f: 120 VAC, 1.1 A , 50/60Hz P: 0.1 KW

Made in Germany   

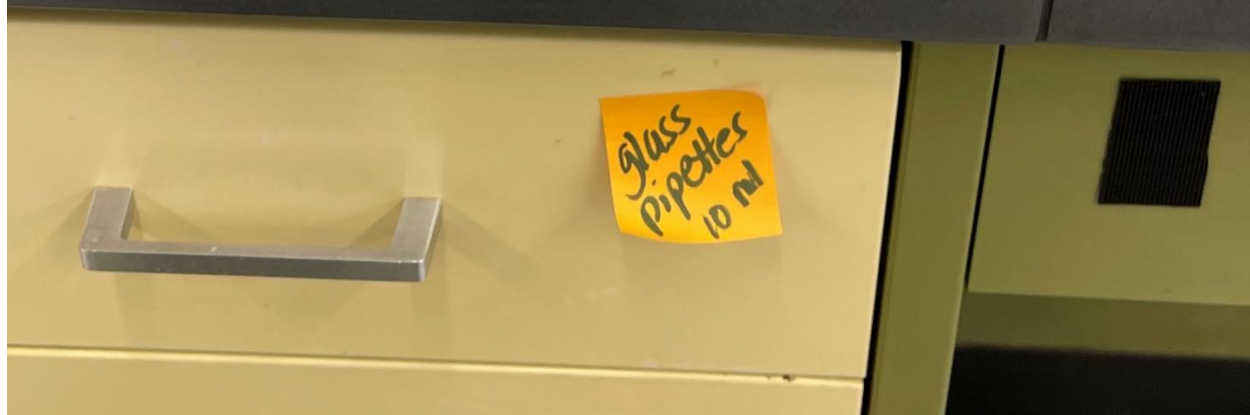



MET
c us
Listing# E112119


Complies with:
UL61010A-1
UL61010A-2-020
CSA C22.2 No. 1010.1
Laboratory Equipment


CLAY ADAMS™ Brand
SERO-FUGE™ 2001
Centrifuge
Serial No. **A583061**

Model 420351
115 VAC ~
2 A
50/60 Hz

Becton Dickinson Primary Care Diagnostics
7 Loveton Circle, Sparks, MD 21152-0370 U.S.A.
CLAY ADAMS, SERO-FUGE, and  are trademarks of Becton Dickinson and Company.
BECTON DICKINSON
MADE IN U.S.A.
10251-1025-102 Rev. 1


169564

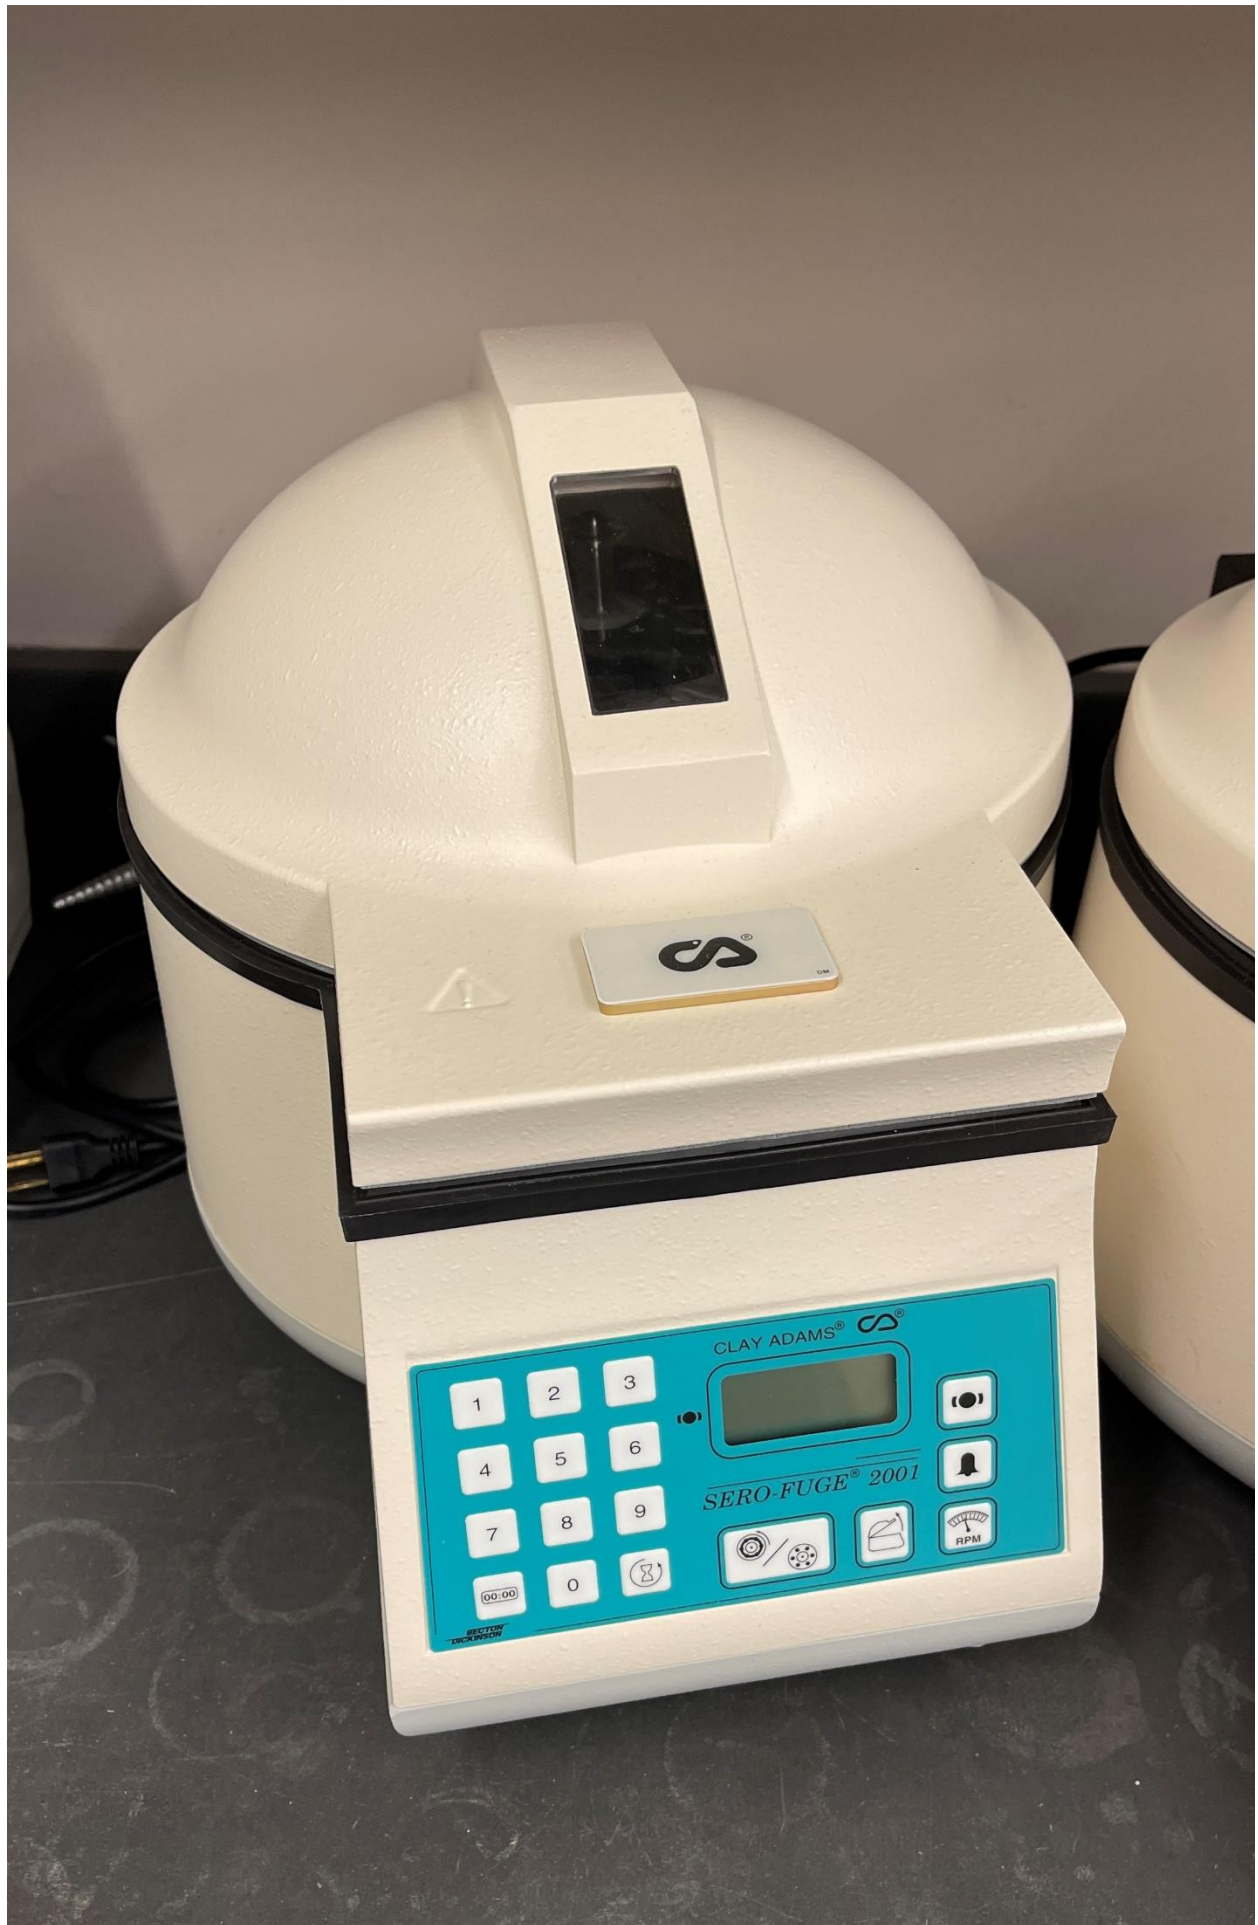

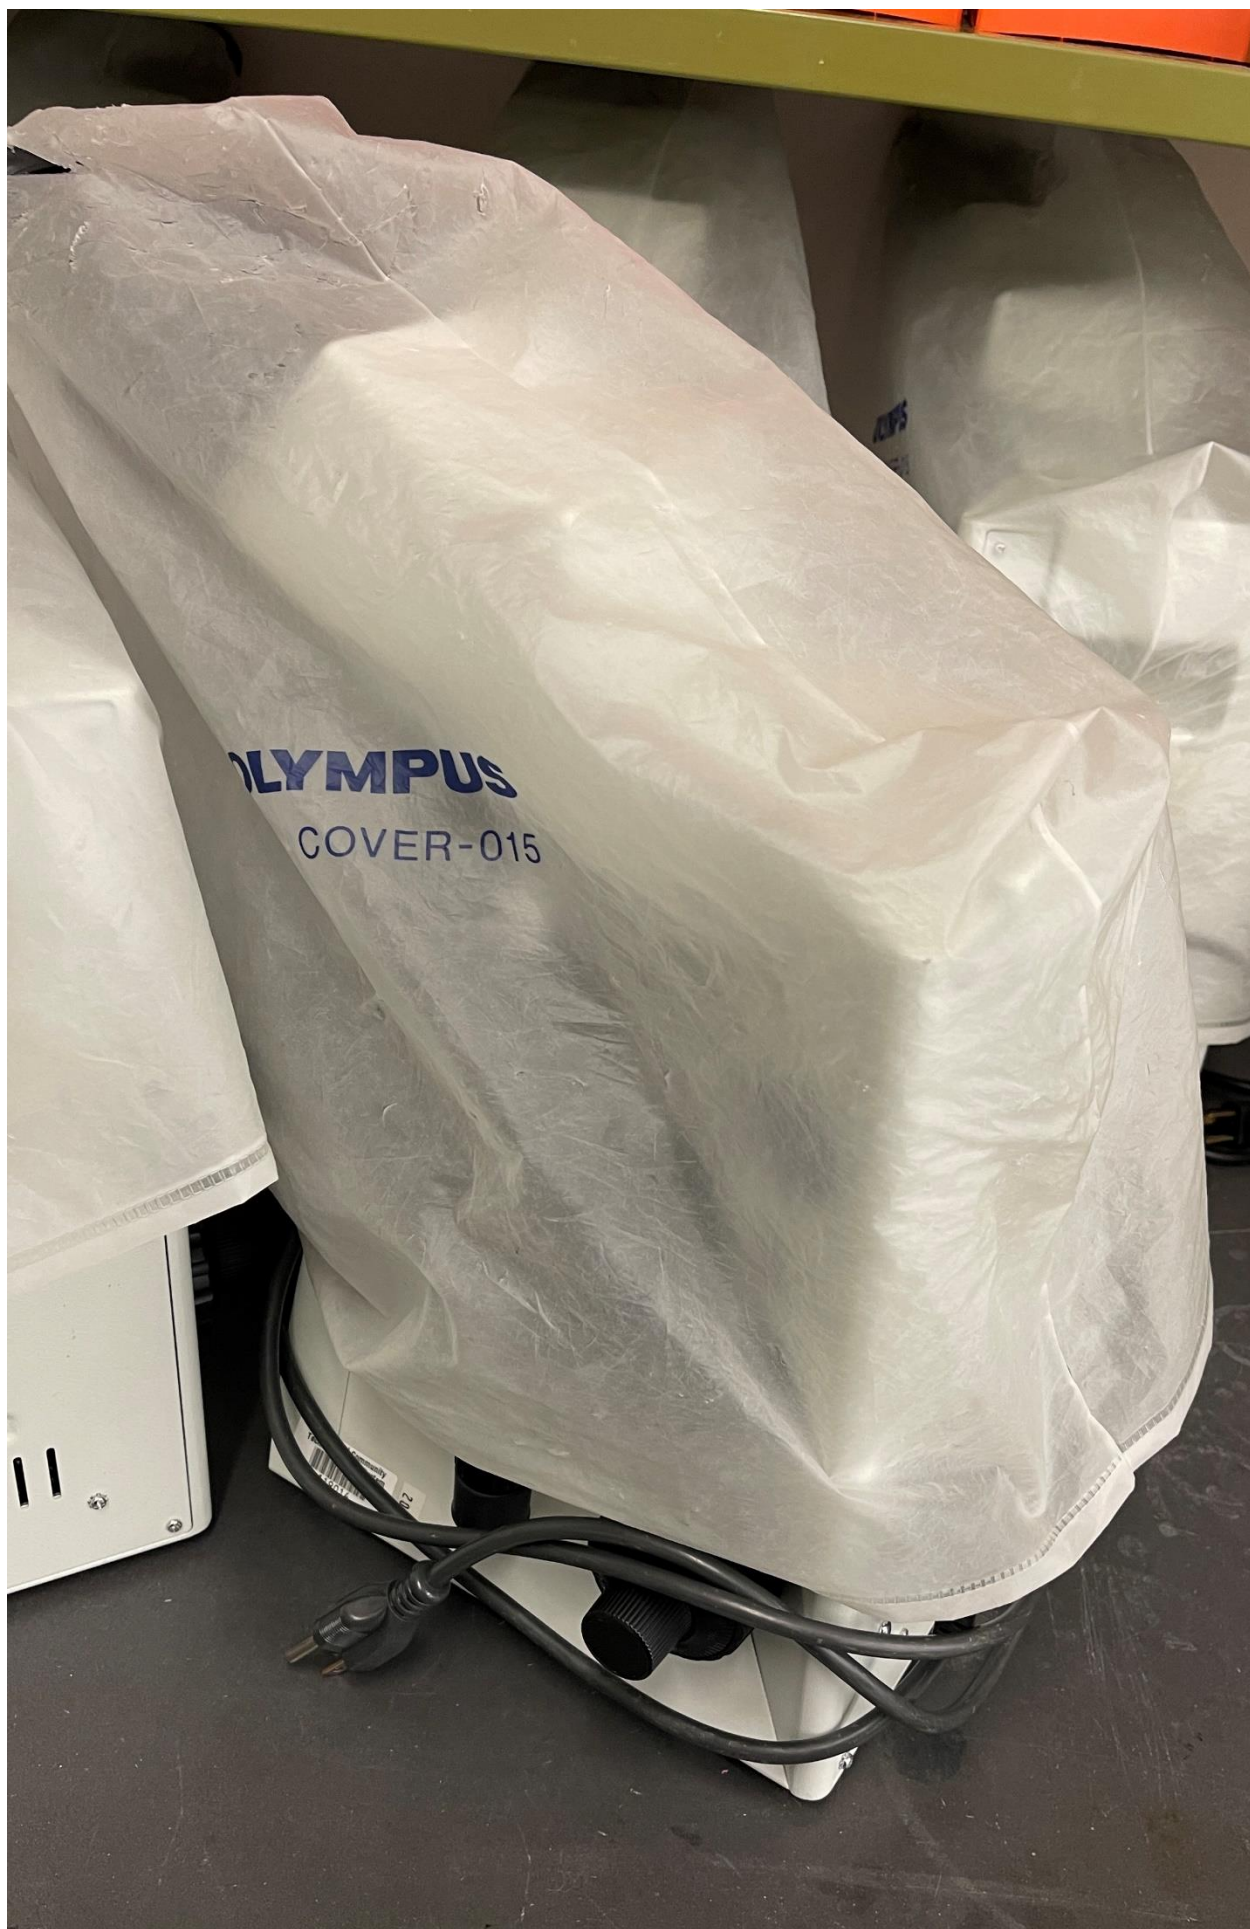

OLYMPUS
COVER-015

MODEL **CX31RBSFA**

100-120/220-240V~
0.85/0.45A 50/60Hz

T2 SN **4M01570**



Laboratory
Equipment
LISTED
8C57




CAUTION

See Manual

OLYMPUS CORPORATION
TOKYO, JAPAN

Made in Philippines

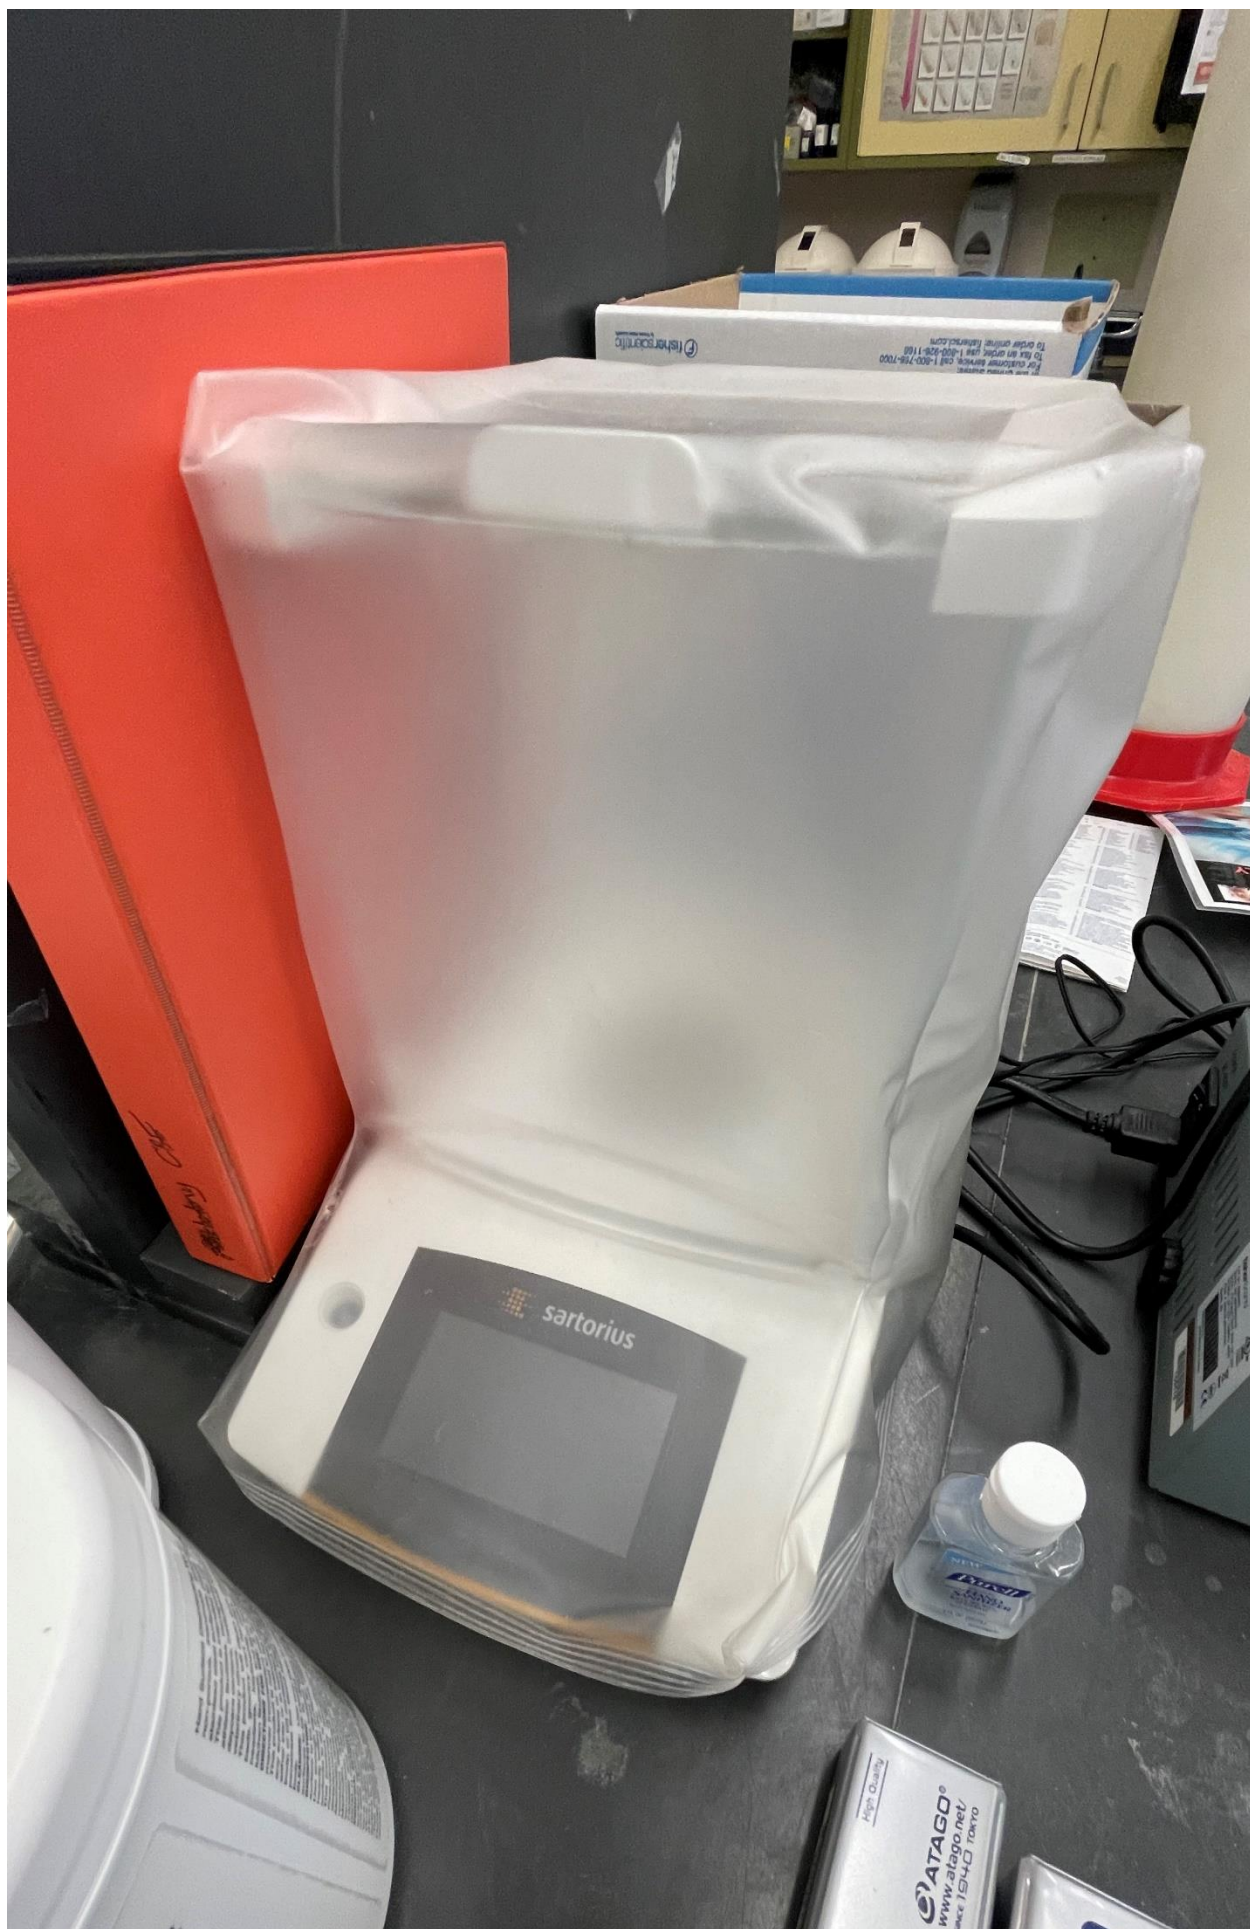



CAUTION: DO NOT INSTALL CLOSER THAN 2
INCHES TO A WALL OF COMBUSTIBLE MATERIAL.
ATTENTION: NE PAS INSTALLER A MOINS DE 2
POUNCES D'UNE PAROI EN MATERIAU COMBUSTIBLE.

Precision Scientific Inc.
3737 West Cortland Street
Chicago, Illinois 60647

COVERED BY ONE OR MORE OF THE FOLLOWING PATENTS: OTHER PATENTS PENDING

CAT. NO.	TEMP.	SERIAL NO.	O.C. LOT
31572-10	70C	108U-1	88544-0085

4EG MODEL	120 VOLTS	200 WATTS	1 PH.	1.7 AMPS	50/60 H.P. HZ.
--------------	--------------	--------------	----------	-------------	-------------------





CO2 INCUBATOR

Forma Scientific

Reset

Over Temp

Water-Jacketed Incubator 3250









